

European Legislation

Electronic Instructions for Use

EU 2021/2226 - Regulation on electronic
instructions for use of medical devices



unitron

This document is provided to you by Unitron Regulatory. It contains the text of the European Union regulation on electronic instructions for use of medical devices (EU) 2021/2226.

unitron Regulatory

Unitron Regulatory is part of Unitron Group. Unitron Group develops and manufactures complete products, such as medical equipment and specific industrial products. This may involve the realisation of a completely new concept, but also the modification and optimisation of existing products. This, in combination with our experience and business strength, will result in a complete business concept. Unitron is active in several markets throughout the world.

Unitron Regulatory is the right partner for product certification in the field of medical devices and life science devices. Our team has specialist knowledge and practical experience with regard to product certification (CE, MDD/MDR, IVDD/IVDR, LVD, FDA, etc.) of medical and life science electronic products and equipment. We are experts in the field of building up a technical product file and product life cycle management from a regulatory perspective.

If you need advice or assistance with the certification of your electronic device or with the interpretation of the MDR text, don't hesitate to contact us.

© 2022 Unitron Group B.V.

Version: 2022/01

All rights reserved. You are free to distribute, copy or print this document or any portion thereof, as long as you intend to support and uphold its purpose to provide the medical device industry with a useful and readable documentation tool. Also, it would be nice if you would honour the work that has been put into it by keeping our name and logo with the document. The digital version is provided free of charge; please don't sell this version.

The text of the EU Regulation on electronic instructions for use of medical devices 2021/2226 is in the public domain.

Designed in the Netherlands. Printed by you. Or given to you by someone else.

www.unitron.nl / www.unitronregulatory.nl

Prefer a digital (hyperlinked) copy? Send a request to regulatory@unitron.nl, and we'll provide it to you free of charge.

Reading guide: [Keyword](#) [Internal reference](#) [External reference](#) [Important date](#)

CONTENTS

Article 1	Introduction	3
Article 2	Definitions	3
Article 3	Electronic instructions for use instead of paper form	3
Article 4	Risk assessment	4
Article 5	Manufacturer obligations	5
Article 6	Providing information to the end user	5
Article 7	Availability through a website	6
Article 8	Notified Body involvement	6
Article 9	Electronic instructions for use in addition to paper form	6
Article 10	Repeal	7
Article 11	Entry into force	7

COMMISSION IMPLEMENTING REGULATION (EU) No 2021/2226

of 14 December 2021

laying down rules for the application of Regulation (EU) 2017/745 of the European Parliament and the Council as regards electronic instructions for use of medical devices

THE EUROPEAN COMMISSION,

Having regard to the Treaty on the Functioning of the European Union,

Having regard to [Regulation \(EU\) 2017/745](#) of the European Parliament and of the Council of 5 April 2017 on medical devices, amending [Directive 2001/83/EC](#), [Regulation \(EC\) No 178/2002](#) and [Regulation \(EC\) No 1223/2009](#) and repealing Council [Directives 90/385/EEC](#) and [93/42/EEC](#) ⁽¹⁾, and in particular Article 5(6) thereof,

Whereas:

- (1) For some medical devices, the provision of instructions for use in electronic form instead of in paper form can be beneficial. It can reduce the environmental burden and reduce costs for the medical device industry while maintaining or improving the level of safety.
- (2) Commission [Regulation \(EU\) No 207/2012](#) ⁽²⁾ has established conditions under which instructions for use of medical devices subject to Council [Directive 90/385/EEC](#) ⁽³⁾ and Council [Directive 93/42/EEC](#) ⁽⁴⁾ could be provided in electronic form instead of in paper form. Both Council Directives have been repealed and replaced by [Regulation \(EU\) 2017/745](#). The rules as regards electronic instructions for use should therefore be adapted to the new requirements of [Regulation \(EU\) 2017/745](#) and technological developments in the field.
- (3) The possibility of providing instructions for use in electronic form instead of in paper form should be limited to certain medical devices and accessories intended to be used under specific conditions. For reasons of safety and efficiency, users should always have the possibility to obtain those instructions for use in paper form upon request.
- (4) In order to reduce potential risks as far as possible, the appropriateness of the provision of instructions for use in electronic form instead of in paper form should be subject to a specific risk assessment by the manufacturer.
- (5) To ensure unconditional access to the instructions for use in electronic form and to facilitate the communication of updates, those instructions should be available on the website of the manufacturer in an official language(s) of the Union determined by the Member State in which the device is made available to the user or patient.
- (6) In order to ensure safety and consistency, instructions for use in electronic form which are provided in addition to instructions for use in paper form should be covered by this Regulation as regards limited requirements in relation to their contents and websites.
- (7) The possibility of providing instructions for use in electronic form should be without prejudice to obligations related to the provision of implant cards in accordance with [Article 18 of Regulation \(EU\) 2017/745](#).
- (8) As the protection of the right to privacy of natural persons with respect to the processing of personal data should be ensured by both manufacturers and notified bodies, it is appropriate to provide that websites containing instructions for use of a medical device fulfil the requirements of [Regulation \(EU\) 2016/679](#) of the European Parliament and of the Council ⁽⁵⁾.
- (9) In order to ensure that the rules as regards electronic instructions for use are adapted to the new requirements of [Regulation \(EU\) 2017/745](#), Commission [Regulation \(EU\) No 207/2012](#) should be therefore repealed. It should however continue to apply to devices placed on the market or put into service during the transitional period set out in [Article 120\(3\) of Regulation \(EU\) 2017/745](#).

- (10) The measures provided for in this Regulation are in accordance with the opinion of the Committee on medical devices,

HAS ADOPTED THIS REGULATION:

Article 1 Introduction

This Regulation [establishes the conditions](#) under which information in the instructions for use, as defined by [Article 2\(14\) of Regulation \(EU\) 2017/745](#) and detailed in [Annex I, Chapter III, point 23.4 to Regulation \(EU\) 2017/745](#) may be provided by manufacturers in electronic form, as referred to in [Annex I, Chapter III, point 23.1\(f\), to Regulation \(EU\) 2017/745](#).

It also establishes [certain requirements](#) concerning contents of and websites for instructions for use that are provided in electronic form in addition to instructions for use in paper form.

This Regulation does not cover products listed in [Annex XVI to Regulation \(EU\) 2017/745](#).

Article 2 Definitions

For the purposes of this Regulation, the following definitions shall apply:

1. ‘[instructions for use in electronic form](#)’ means instructions for use displayed in electronic form by the device, contained in portable electronic storage media supplied by the manufacturer together with the device, or made available through a software or a website;
2. ‘[professional users](#)’ means persons using the medical device in the course of their work in the framework of a professional healthcare activity;
3. ‘[fixed installed medical devices](#)’ means devices and their accessories which are intended to be installed, fastened or otherwise secured at a specific location in a health institution so that they cannot be moved from this location or detached without using tools or apparatus, and which are not specifically intended to be used within a mobile healthcare institution.

Article 3 Electronic instructions for use instead of paper form

1. Manufacturers may provide instructions for use in electronic form instead of in paper form where those instructions relate to any [of the following devices](#):
 - (a) [implantable](#) and [active implantable medical devices](#) and their accessories covered by [Regulation \(EU\) 2017/745](#);
 - (b) [fixed installed medical devices](#) and their accessories covered by [Regulation \(EU\) 2017/745](#);
 - (c) [medical devices](#) and their accessories covered by [Regulation \(EU\) 2017/745](#) and [fitted with](#) a built-in system visually displaying the instructions for use.
2. Manufacturers may provide instructions for use in electronic form instead of in paper form for the devices listed in paragraph 1 under [the following conditions](#):
 - (a) the devices and accessories are intended for [exclusive use by professional users](#); and
 - (b) the use by other persons is [not reasonably foreseeable](#).
3. For [software](#) covered by [Regulation \(EU\) 2017/745](#), manufacturers may provide instructions for use in electronic form by means of the software itself instead of in paper form.

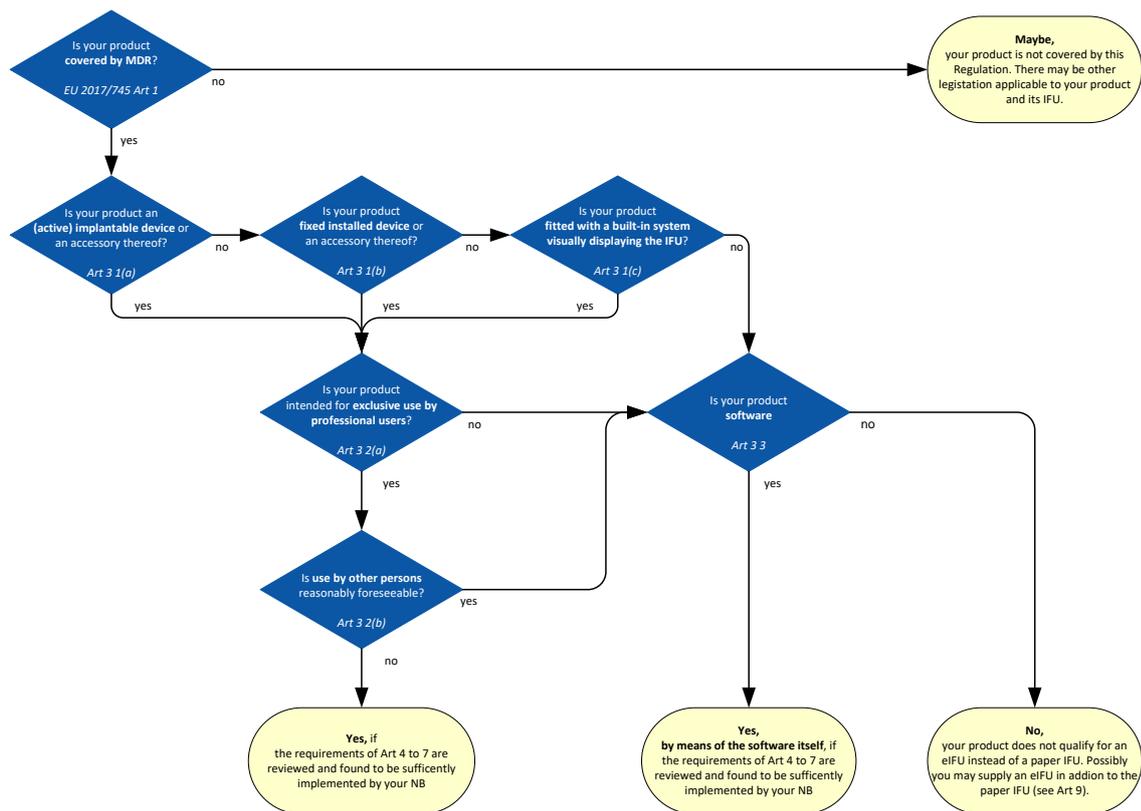


Figure 1 - qualification helper for an electronic IFU instead of a paper IFU

Article 4 Risk assessment

1. Manufacturers of devices referred to in [Article 3](#), paragraphs 1 and 3, that provide instructions for use in electronic form instead of in paper form shall undertake a [documented risk assessment](#) which shall cover at least the following elements:
 - (a) [knowledge and experience of the intended users](#) in particular regarding the use of the device and user needs;
 - (b) characteristics of the [environment](#) in which the device will be used;
 - (c) knowledge and experience of the intended user of the [hardware and software needed](#) to display the instructions for use in electronic form;
 - (d) [access of the user](#) to the reasonably foreseeable electronic resources needed at the time of use;
 - (e) [performance of safeguards](#) to ensure that the electronic data and content are protected from tampering;
 - (f) [safety and back-up mechanisms](#) in the event of a hardware or software fault, particularly if the instructions for use in electronic form are integrated within the device;
 - (g) [foreseeable medical emergency situations](#) requiring the provision of information in paper form;
 - (h) [impact caused by the temporary unavailability](#) of the specific website or of the Internet in general, or of their access in the healthcare facility as well as the safety measures available to cope with such a situation;
 - (i) evaluation of the [time period](#) within which the instructions for use shall be provided in paper form at the user's request;
 - (j) assessment of [the website's compatibility displaying the electronic instructions](#) for use with different devices which could be used to display those instructions;
 - (k) management of different versions of the instructions for use, where applicable in accordance with [Article 5](#)(8).
2. The risk assessment for the provision of the instructions for use in electronic form shall be [updated](#) in view of the experience gained in the post-marketing phase.

Article 5 Manufacturer obligations

Manufacturers of devices referred to in [Article 3](#), paragraphs 1 and 3, may provide instructions for use in electronic form instead of in paper form under the following conditions:

1. the risk assessment referred to in [Article 4](#) shall demonstrate that providing instructions for use in electronic form [maintains or improves the level of safety](#) obtained by providing the instructions for use in paper form;
2. they shall provide instructions for use in electronic form [in all Member States](#) where the product is made available or put into service, unless duly justified in the risk assessment referred to in [Article 4](#);
3. they shall have a system in place to [provide](#) the instructions for use [in printed paper form](#) at no additional cost for the user, within the time period set out in the risk assessment referred to in [Article 4](#) and at the latest within 7 calendar days of receiving a request from the user or at the time of delivery of the device if so requested at the time of order;
4. they shall [provide](#), on the device or on a leaflet, [information on foreseeable medical emergency situations](#) and, for devices fitted with a built-in system visually displaying the instructions for use, [information on how to start the device](#);
5. they shall [ensure the proper design and functioning](#) of the instructions for use in electronic form and provide verification and validation evidence to this effect;
6. for medical devices fitted with a built-in system visually displaying the instructions for use, they shall [ensure](#) that displaying the instructions for use [does not impede the safe use](#) of the device, in particular life-monitoring or life-supporting functions;
7. they shall [provide](#), in their catalogue or in other appropriate device information support, [information on software and hardware requirements](#) needed to display the instructions for use;
8. they shall [have a system](#) in place to clearly [indicate](#) when the instructions for use have been [revised](#) and to [inform](#) each user of the device thereof if the revision was necessary for safety reasons;
9. for devices [with a defined expiry date](#), except implantable devices, they shall [keep](#) the instructions for use [available](#) for the users in electronic form for at least 2 years after the end of the expiry date of the last produced device;
10. for devices [without a defined expiry date](#) and for [implantable devices](#), they shall [keep](#) the instructions for use [available](#) for the users in electronic form for a period of 15 years after the last device has been placed on the market.
11. the instructions for use [shall be available on their website](#) in an official language of the Union determined by the Member State in which the device is made available to the user or patient;
12. effective systems and procedures shall be in place [to ensure that device users](#) having downloaded instructions for use from the website [can be informed in case of updates](#) or corrective actions with regards to those instructions for use;
13. all issued historical electronic versions of the instructions for use shall be available on the website.

Article 6 Providing information to the end user

1. Manufacturers shall clearly [indicate](#) on the label that the instructions for use of the device are supplied in electronic form instead of in paper form.
That information shall be provided [on the packaging](#) for each unit or, where appropriate, on the sales packaging. In the case of fixed installed medical devices, that information shall also be provided [on the device](#) itself.
In the case of software, the information shall be provided at the location from where access to the software is granted.
2. Manufacturers shall [provide information on how to access](#) the instructions for use in electronic form.
That information shall be provided as set out in the second subparagraph of paragraph 1 or, if not practicable, [in a paper document](#) supplied with each device.
3. The information on how to access the instructions for use in electronic form shall [contain](#) the following:
 - (a) any information needed to view the instructions for use;

- (b) the Basic UDI-DI and/or the UDI-DI of the device, as respectively referred to in [Article 27\(6\)](#) and [Article 27\(1\), point \(a\)\(i\), of Regulation \(EU\) 2017/745](#), and any additional information allowing the identification of the device, including its name and if applicable the model;
 - (c) relevant manufacturer contact details e.g. manufacturer's name, address, email address or other means of online communication and website;
 - (d) where and how instructions for use in paper form can be requested and within which time they shall be obtained at no additional cost in conformity with [Article 5](#), point (3).
4. Where, for devices and accessories referred to in [Article 3\(1\)](#), point (a), a part of the instructions for use is intended to be [provided to the patient](#), that part shall [not be provided in electronic form](#).
5. The instructions for use in electronic form shall [be available entirely as text](#) which may contain symbols and graphics with at least the same information as the instructions for use in paper form. Video or audio files may be provided in addition to the text.

Article 7 Availability through a website

1. Where manufacturers provide the instructions for use in electronic form on an electronic storage medium together with the device or where the device itself is fitted with a built-in system visually displaying the instructions for use, the instructions for use in electronic form shall also be made accessible - to the users [through a website](#).
2. Any website containing instructions for use of a device which are provided in electronic form instead of in paper form shall comply with the following requirements:
- (a) the instructions for use shall be provided in [a commonly used format](#) that can be read with freely available software;
 - (b) it shall be [protected](#) against [unauthorised access and tampering of content](#) in accordance with [Article 4\(1\)](#), point (e);
 - (c) it shall be provided in such a way that the server [downtime](#) and display [errors](#) are [reduced](#) as far as possible;
 - (d) it shall [fulfil the requirements](#) of [Regulation \(EU\) 2016/679](#);
 - (e) the Internet address as displayed in accordance with [Article 6\(2\)](#) shall be [stable and directly accessible](#) during the periods set out in [Article 5](#), points (9) and (10);
 - (f) all [previous versions](#) of the instructions for use issued in electronic form and their date of publication shall be [available](#) on the website.

Article 8 Notified Body involvement

Where applicable, the [fulfilment of the obligations laid down in Articles 4 to 7](#) of this Regulation shall be reviewed by a notified body during the procedure applicable for conformity assessment as referred to in [Article 52 of Regulation \(EU\) 2017/745](#).

Article 9 Electronic instructions for use in addition to paper form

Instructions for use in electronic form, which are provided [in addition](#) to complete instructions for use in paper form, shall be [consistent with the content](#) of the instructions for use in paper form.

Where such instructions for use are provided through a website, this website shall fulfil the requirements set out in [Article 7\(2\)](#), points (b), (d) and (f).

Article 10 Repeal

Commission [Regulation \(EU\) No 207/2012](#) is repealed.

However, it shall continue to apply to devices placed on the market or put into service in accordance with [Article 120\(3\) of Regulation \(EU\) 2017/745](#) until **26 May 2024**.

References to [Regulation \(EU\) No 207/2012](#) shall be construed as references to this Regulation and read in accordance with the correlation table in the Annex.

Article 11 Entry into force

This Regulation shall enter into force on the twentieth day following that of its publication in the Official Journal of the European Union. Being, **4 January 2022**.

Note: publication [Official Journal of the European Union, L 448/32, 15 December 2021](#)

This Regulation shall be binding in its entirety and directly applicable in all Member States.

Done at Brussels, **14 December 2021**.

ANNEX

Correlation table

Commission Regulation (EU) No 207/2012	This Regulation
Article 1	Article 1
Article 2	Article 2
Article 3(1)	Article 3(1)
Article 3(2)	Article 3(2)
-	Article 3(3)
Article 4	Article 4
Article 5	Article 5
Article 6	Article 6
Article 7	Article 7
Article 8	Article 8
Article 9	Article 9
-	Article 10
Article 10	Article 11